



## Effect of Different Implant Angulation on Stresses Transmitted by Fixed Detachable Prosthesis in All-on-Four Concept (In-vitro study)

Eslam Abdelwahab Ahmed Dawood\*, Fadel Elsaid Abdelfattah<sup>1</sup>,  
Nahed Ahmed Kamel Kashef<sup>2</sup>

1,2. BDS, MSc, PhD Professor, Prosthodontic department, Faculty of dentistry, Tanta University, Elgeish st. Tanta, Egypt.

**Corresponding Author: Eslam Abdelwahab Ahmed Dawood**, Assistant lecturer, Prosthodontic department, Faculty of dentistry, Tanta University, Elgeish st. Tanta, Egypt.

**Copy Right:** © 2021 Eslam Abdelwahab Ahmed Dawood. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

**Received Date: June 09, 2021**

**Published date: July 01, 2021**

### Abstract

**Background:** The objective of this study was to compare between stress produced by maxillary fixed-detachable prosthesis around the implants placed with different angulations following All-On-Four Concept.

**Methods:** For this study, two standardized maxillary epoxy models were made, surgical guides were fabricated by CAD/CAM according to desired angulations. Two groups were designed, for the group, A implants were inserted following the All-On-Four concept with 45 degrees distal angulation of distal implants while for Group B implants were inserted following the All-On-Four concept with 30 degrees distal angulation of distal implants.

The fixed detachable prosthesis was made for 2 groups by plastic castable abutments and casting procedure. After that, a strain gauge was installed around implants in buccal, palatal, mesial and distal aspects, and a load of 100N was applied vertically and another load of 65N was applied obliquely by digitalized testing machine upon occlusal plate 10 times.

**Results:** There was a significant difference between posterior implants tilted by 45 degrees and posterior implants tilted by 30 degrees under vertical and oblique load without taking into consideration the effect of the cantilever. The anterior implants are significantly less subjected to stresses than posterior tilted implants. An oblique load has generated higher stresses than vertical loads overall implants. **Conclusions:** Within the limitations of this in-vitro study, it can be concluded that with short cantilever implant-supported prosthesis avoiding the increase in the tilt of implants more than 30 degrees is recommended to decrease stresses transmitted to surrounding structures around both anterior and posterior implants. Off axial loads will generate more stresses around implants.

**Keywords:** All-On-Four, Dental Implants, Tilted Implants, Fixed Detachable Prosthesis, Strain Gauge Analysis.

## Introduction

The use of endo-osseous dental implants is a well-accepted and encouraging treatment modality for the rehabilitation of partially or completely edentulous patients. Although the success rate with implants is high, biological, and technical complications around the implants are reported. In recent years, oral implantology has undergone a well-deserved innovation and dental implants are now considered the preferred treatment plan in an increasing number of carefully selected cases (1,2).

In many cases, the treatment of the edentulous maxilla is more challenging and requires more elective procedures than are necessary for the mandible, particularly concerning the following criteria (3,4): degree of atrophy of the residual jaw, location of the implants, tilting the axis of the implants, soft and hard tissue volume, facial profile, esthetics, function and phonetics.

In recent years, it has been proposed to use inclined implants to restore edentulous maxillary and mandibular jaws. Implants of regular length can be placed, allowing as much cortical bone engagement as possible, thereby increasing initial stability (5).

The All-on-Four concept is designed to maximize the use of available residual bone in atrophic jaws. Therefore, it allows for immediate effect and avoids regenerative procedures that increase treatment costs and patient morbidity as well as the complications inherent in these procedures. All-on-Four treatment ideas provide predictable results in the treatment of atrophic jaws. The evidence provided shows a promising prognosis for the treatments. The results showed that the survival rate of prostheses and implants was high after three years of follow-up. There are no statistically significant differences in clinical results between the upper and lower dental arches and the axial and oblique implants (6-8).

The stresses transferred from dental implants to surrounding bone are affected by many factors such as the sort of loading, the bone-implant interface, the length and diameter of the implants, the implant shape, structure of the implant surface, the superstructure and also the quality and the quantity of the encircling bone (9). Biomechanical analyses indicate that the foremost anterior and posterior implants supporting a reconstruction take the main load share at cantilever loading, regardless of the quantity of intermediate implants (6).

After osseointegration is achieved; long-term clinical follow-ups reported biological or mechanical complications (10,11). The factors that affect the prognosis of dental implants should be carefully considered before attempting to rehabilitate the patients with implants. These factors are periodontally compromised patients, age, bone density, occlusion, smoking, genetics, systemic diseases, microorganisms, antibiotics, and type of implants (12).

A strain gauge is a device used to measure the strain of the object. The most common type of strain gauge consists of an insulating flexible backing that supports a metallic foil pattern. The gauge is attached to the object by a suitable adhesive. As the object is deformed, the foil is deformed, causing its electrical resistance to change (13-15).

In this in-vitro study strain gauge technology has been used to measure micro strains induced by maxillary fixed detachable dental prosthesis supported by implants using the All-On-Four treatment concept with different angulations.

## **Material & Methods**

Approval for this research was obtained from the Faculty of Dentistry, Tanta University, and the Research Ethics Committee (REC). The design and procedures of the present study were accomplished according to the research guidelines published by the (REC) Faculty of Dentistry, Tanta University.

Two identical ready-made maxillary completely edentulous epoxy resin models covered by 2 mm of silicon resilient material to simulate oral mucosa were used for this study. The two models were divided into two groups as follows: Group (A): Fixed detachable dental prosthesis has been fabricated to fit on four implants using the All-On-Four concept. The two anterior implants were placed vertically, while the

two posterior implants were placed at distal angulation of 45 degrees. Group (B): Fixed detachable dental prosthesis has been fabricated to fit on four implants using the All-On-Four concept. The two anterior implants were placed vertically, and the two posterior implants were placed at distal angulation of 30 degrees.

**Implant installation:**

A rubber base impression was taken for the epoxy model then the impression was poured with hard dental stone to produce the stone cast needed for fabrication of trial denture base from self-cure acrylic resin. After that set of artificial acrylic, teeth were done upon trial denture base to determine the exact location of teeth. Radiographic markers (gutta-percha) were placed upon trial denture in palatal and buccal holes 1 mm deep and 1.5 mm wide at the canine and first molar region to make radiographic stent then Cone Beam Computer Tomography was taken once for radiographic stent alone and another one for model and stent together. Implant planning was done using 3Diemme Real Guide Software according to the position of teeth determined by the radiographic stent, the 2 anterior implants were planned axially in the canine region. The two posterior implants in the model are tilted by 450 degrees in the second premolar region while in the second model the posterior implants were tilted by 300degrees also in the second premolar region. Two Surgical guides were 3D Printed, checked on corresponding models for adaptation and accuracy.

Fixation of the surgical guides on the corresponding model was done after being sure that the surgical guides are seated properly on both models. A tissue punch was used to remove the area of the silicon layer at the drilling site. Drilling was performed by using Biohorizons guided drilling kit using the green key and a full sequence of drilling burs to the selected implant size was used.

For both models four holes were drilled, two in canine regions with 10 mm depth, and two in second premolar regions with 15 mm in depth on both sides. The Implants were selected from the Biohorizons implant system, two implants measuring 3.8 mm diameter and 10 mm length were inserted in the canine region, and two implants system measuring 3.8 mm diameter and 15 mm length were inserted in the second premolar region in both models. The implants were inserted in the prepared sites and rotated clockwise with a torque equals to 40 N. Complete implant insertion till the implant becomes flushed with the epoxy resin model.

After implant placement was checked, from the connection set of Biohorizons, straight multiunit abutments were tightened to anterior implants while 300 angled multiunit abutments were tightened to posterior implants to achieve Parallelism between the abutment and ensure the passive fit of the prosthesis. Plastic custom castable coping with hex driver was attached to anterior and posterior multiunit abutments. Waxing up for metallic framework connecting four castable coping was done for both models. After that casting, the wax-up was done using a casting machine to produce a metallic

framework. The waxed framework was then spread in the casting ring. Then Casting ring was inserted into the casting machine to produce a metallic framework.

Metallic frameworks were checked on the model to ensure passive fit, then a thin layer of metal opaquer was placed over the metallic framework to mask the dark shade of metal. Later, overlay porcelain made by conventional technique and contain holes for screws to attach the prosthesis to abutments was fabricated, finished, and polished. Every prosthesis consists of twelve teeth ending with the first molar teeth with fixed cantilever length in both restorations.

#### **Fabrication of occlusal plate for load application:**

The occlusal plate has been fabricated by making waxing up on the occlusal surface of the fixed detachable prosthesis so that the wax-up takes the shape of the occlusal surface of the prosthesis and adapted on it. After finishing the wax-up, it was placed in a casting machine and cast into a metal plate which has one surface occluding with the prosthesis and another flat surface. A flat metal plate is placed on top of the occlusal plate to apply load upon it.

#### **Installation of strain gauge:**

The strain gauges were used for this study with the specification according to the manufacture: For each model four tunnels (3 mm in depth, 4 mm in width and 5 mm in length) were prepared at the top of the epoxy resin model just around the implant surface parallel to the long axis of the implant in mesial, distal, buccal and lingual surfaces, four strain gauges installed in each tunnel in the epoxy resin on the surface which was toward the implants to measure the micro strains in the medium surrounding the implant in model A and model B.

A strain gauge adhesive was used to cement the strain gauges on the epoxy resin parallel to the long axis of the implant and held in their sites for 5 minutes. And the wires of the strain gauges were connected to a digital multichannel strainmeter. The strainmeter was connected to a compatible laptop containing the meter control software (EDX 10A).

Each of the two models placed on the base of the loading device of the universal testing machine and then before running the test, the occlusal plate was put on the occlusal surface of the prosthesis then the strainmeter was balanced to zero. The point of load application was the center of the occlusal plate. The forces were delivered to the flat surface of the occlusal plate using a loading pin (applicator) attached to the digitalized testing machine. Both were placed with the fixed detachable prosthesis in its place in a horizontal plane of the base of the loading device base and bilateral static 100 N vertical load was applied. Also, both models were placed with the fixed detachable prosthesis in its place on the surface of an oblique wooden segment which made the angle equal 35o with the applied load and bilateral static

65 N oblique load was applied. The load is applied 10 times for each model vertically and obliquely to ensure the reproducibility of the results with at least 5 minutes interval between the readings to allow relief of formed strains before making the next reading.

**Statistical analysis:**

The microstrain data were collected of the present study was collected and tabulated and statistically analyzed using the mean, standard deviation, and Student t-test to compare the mean of post-load values between two groups. Statistical analysis was performed by using SPSS program version 20 (SPSS Inc. Chicago, USA).

**Results**

The results showed the mean and standard deviation of the values recorded from the four strain gauges at the buccal, lingual, mesial, and distal around each implant under bilateral 100 N vertical load and 65 N oblique load for Groups.

|                        | Group   |   |        |         |   |       | T-Test |         |
|------------------------|---------|---|--------|---------|---|-------|--------|---------|
|                        | Group A |   |        | Group B |   |       | t      | P-value |
|                        | Mean    | ± | SD     | Mean    | ± | SD    |        |         |
| <b>Vertical IMP AR</b> | 39.051  | ± | 5.752  | 37.726  | ± | 8.016 | 0.425  | 0.676   |
| <b>Vertical IMP AL</b> | 41.566  | ± | 9.781  | 38.204  | ± | 8.423 | 0.824  | 0.421   |
| <b>Differences</b>     | -2.515  | ± | 13.148 | -0.478  | ± | 9.776 |        |         |
| <b>Paired Test</b>     | 0.560   |   |        | 0.881   |   |       |        |         |

**Table (1):** Mean ±SD of microstrains around implants in both groups (**regarding anterior implants under vertical load**)

**From table (1) which compared both the groups regarding anterior implants under vertical load, it was founded that:**

- 1- In group A there is no significant difference between right and left anterior implants under vertical load

2- In group B there is no significant difference between right and left anterior implants under vertical load

3- Comparing between both groups under vertical load, it is concluded that there is no significant difference between both groups at both right and left implants

|                        | Group   |   |        |         |   |       | T-Test |         |
|------------------------|---------|---|--------|---------|---|-------|--------|---------|
|                        | Group A |   |        | Group B |   |       | t      | P-value |
|                        | Mean    | ± | SD     | Mean    | ± | SD    |        |         |
| <b>Vertical IMP PR</b> | 55.307  | ± | 14.573 | 43.612  | ± | 5.859 | 2.355  | 0.030*  |
| <b>Vertical IMP PL</b> | 57.997  | ± | 12.524 | 43.805  | ± | 4.434 | 3.378  | 0.003*  |
| <b>Differences</b>     | -2.690  | ± | 21.894 | -0.193  | ± | 8.490 |        |         |
| <b>Paired Test</b>     | 0.707   |   |        | 0.944   |   |       |        |         |

**Table (2):** Mean ±SD of microstrains around implants in both groups (regarding posterior implants under vertical load):

**From table (2) which compared between both groups regarding posterior implants under vertical load, it was founded that:**

1- In group A there is no significant difference between right and left posterior implants under vertical load.

2- In group B there is no significant difference between right and left posterior implants under vertical load.

3- it is founded that there is a significant difference between both groups under vertical load at both right and left posterior implants with higher values assigned to Group A.

|                           | Group   |   |       |         |   |       | T-Test |         |
|---------------------------|---------|---|-------|---------|---|-------|--------|---------|
|                           | Group A |   |       | Group B |   |       | t      | P-value |
|                           | Mean    | ± | SD    | Mean    | ± | SD    |        |         |
| <b>Vertical Anterior</b>  | 40.308  | ± | 4.601 | 37.964  | ± | 6.611 | 0.920  | 0.370   |
| <b>Vertical Posterior</b> | 56.651  | ± | 8.049 | 43.709  | ± | 2.995 | 4.765  | <0.001* |
| <b>Differences</b>        | -16.343 | ± | 8.095 | -5.745  | ± | 7.040 |        |         |
| <b>Paired Test</b>        | <0.001* |   |       | 0.030*  |   |       |        |         |

**Table (3):** Mean ±SD of microstrains around implants in both groups (**regarding anterior and posterior implants under vertical load**):

**Comparing both groups at anterior and posterior implants under vertical load is shown in table (3) as follow:**

- 1- In group A there is a significant difference between anterior and posterior implants under vertical load.
- 2- In Group B there is a significant difference between anterior and posterior implants under vertical load.
- 3- Comparing both groups shows a significant difference between posterior implants, while there is no significant difference between anterior implants under vertical load.

|                       | Group   |   |        |         |   |        | T-Test |         |
|-----------------------|---------|---|--------|---------|---|--------|--------|---------|
|                       | Group A |   |        | Group B |   |        | t      | P-value |
|                       | Mean    | ± | SD     | Mean    | ± | SD     |        |         |
| <b>Oblique IMP AR</b> | 46.005  | ± | 12.504 | 41.347  | ± | 13.365 | 0.805  | 0.431   |
| <b>Oblique IMP AL</b> | 48.657  | ± | 12.589 | 41.025  | ± | 15.515 | 1.208  | 0.243   |
| <b>Differences</b>    | -2.652  | ± | 20.018 | 0.322   | ± | 25.055 |        |         |
| <b>Paired Test</b>    | 0.685   |   |        | 0.968   |   |        |        |         |

**Table (4):** Mean ±SD of microstrains around implants in both groups (**regarding anterior implants under oblique load**):

**Comparing both groups regarding anterior implants under oblique load is shown in table (4) as follow:**

- 1- In group A there is no significant difference between right and left anterior implants under oblique load.
- 2- In group B there is no significant difference between right and left anterior implants under oblique load.
- 3- It is founded that there is no significant difference when comparing both groups at right and left anterior implants under oblique load.

|                       | Group   |   |        |         |   |        | T-Test |         |
|-----------------------|---------|---|--------|---------|---|--------|--------|---------|
|                       | Group A |   |        | Group B |   |        | t      | P-value |
|                       | Mean    | ± | SD     | Mean    | ± | SD     |        |         |
| <b>Oblique IMP PR</b> | 65.998  | ± | 18.741 | 51.530  | ± | 11.366 | 2.087  | 0.051*  |
| <b>Oblique IMP PL</b> | 68.826  | ± | 17.912 | 54.266  | ± | 13.100 | 2.075  | 0.053*  |
| <b>Differences</b>    | -2.828  | ± | 26.403 | -2.736  | ± | 18.374 |        |         |
| <b>Paired Test</b>    | 0.743   |   |        | 0.649   |   |        |        |         |

**Table (5): Mean ±SD of microstrains around implants in both groups (regarding posterior implants under oblique load):**

**Comparing both groups regarding posterior implants under oblique load shown in table (5) which is:**

- 1- In group A there is no significant difference between right and left posterior implants under oblique load.
- 2- In group B there is no significant difference between right and left posterior implants under oblique load.
- 3- Comparing between two groups at right and left posterior implants under oblique load, it is founded that there is a significant difference between the implants with high values assigned to Group A.

|                          | Group          |          |               |                |          |               | T-Test       |               |
|--------------------------|----------------|----------|---------------|----------------|----------|---------------|--------------|---------------|
|                          | Group A        |          |               | Group B        |          |               | t            | P-value       |
|                          | Mean           | ±        | SD            | Mean           | ±        | SD            |              |               |
| <b>Oblique Anterior</b>  | <b>47.331</b>  | <b>±</b> | <b>7.566</b>  | <b>41.186</b>  | <b>±</b> | <b>7.261</b>  | <b>1.853</b> | <b>0.080</b>  |
| <b>Oblique Posterior</b> | <b>67.412</b>  | <b>±</b> | <b>12.719</b> | <b>52.898</b>  | <b>±</b> | <b>8.124</b>  | <b>3.041</b> | <b>0.007*</b> |
| <b>Differences</b>       | <b>-20.081</b> | <b>±</b> | <b>16.136</b> | <b>-11.712</b> | <b>±</b> | <b>13.249</b> |              |               |
| <b>Paired Test</b>       | <b>0.003*</b>  |          |               | <b>0.021*</b>  |          |               |              |               |

**Table (6):** Mean ±SD of microstrains around implants in both groups (**regarding anterior and posterior implants under oblique load**):

**Comparing both groups at anterior and posterior implants under oblique load in the table (6) showed that:**

- 1- In group A, there was no significant difference between the anterior implants under oblique load between both groups.
- 2- In group B, there was a significant difference between posterior implants under oblique load between both groups.
- 3- Comparing both groups under oblique load, it is founded that there is no significant difference at anterior implants while there is a significant difference at posterior implants.

|                          | Group         |          |              |               |          |              | T-Test       |              |
|--------------------------|---------------|----------|--------------|---------------|----------|--------------|--------------|--------------|
|                          | Group A       |          |              | Group B       |          |              | t            | P-value      |
|                          | Mean          | ±        | SD           | Mean          | ±        | SD           |              |              |
| <b>Vertical Anterior</b> | <b>40.308</b> | <b>±</b> | <b>4.601</b> | <b>37.964</b> | <b>±</b> | <b>6.611</b> | <b>0.920</b> | <b>0.370</b> |
| <b>Oblique Anterior</b>  | <b>47.331</b> | <b>±</b> | <b>7.566</b> | <b>41.186</b> | <b>±</b> | <b>7.261</b> | <b>1.853</b> | <b>0.080</b> |
| <b>Differences</b>       | <b>-7.023</b> | <b>±</b> | <b>9.541</b> | <b>-3.222</b> | <b>±</b> | <b>3.921</b> |              |              |
| <b>Paired Test</b>       | <b>0.045*</b> |          |              | <b>0.029*</b> |          |              |              |              |

**Table (7):** Mean ±SD of microstrains around implants in both groups (**regarding anterior implants under vertical and oblique load**):

**Comparing between vertical and oblique forces between both groups is shown in table (7) and showed that:**

- 1- There is a significant difference between vertical and oblique loads between anterior implants in Group A.
- 2- There is a significant difference between vertical and oblique loads between anterior implants in Group B.
- 3- There is no significant difference between both groups under both vertical and oblique loads regarding anterior implants.

|                           | Group          |          |               |               |          |              | T-Test       |                   |
|---------------------------|----------------|----------|---------------|---------------|----------|--------------|--------------|-------------------|
|                           | Group A        |          |               | Group B       |          |              | t            | P-value           |
|                           | Mean           | ±        | SD            | Mean          | ±        | SD           |              |                   |
| <b>Vertical Posterior</b> | <b>56.651</b>  | <b>±</b> | <b>8.049</b>  | <b>43.709</b> | <b>±</b> | <b>2.995</b> | <b>4.765</b> | <b>&lt;0.001*</b> |
| <b>Oblique Posterior</b>  | <b>67.412</b>  | <b>±</b> | <b>12.719</b> | <b>52.898</b> | <b>±</b> | <b>8.124</b> | <b>3.041</b> | <b>0.007*</b>     |
| <b>Differences</b>        | <b>-10.761</b> | <b>±</b> | <b>15.350</b> | <b>-9.189</b> | <b>±</b> | <b>9.026</b> |              |                   |
| <b>Paired Test</b>        | <b>0.054*</b>  |          |               | <b>0.011*</b> |          |              |              |                   |

**Table (8): Mean ±SD of microstrains around implants in both groups (regarding anterior implants under vertical and oblique load):**

**Comparing between vertical and oblique forces between both groups is shown in table (8) and showed that:**

- 1- There is a significant difference between vertical and oblique loads between posterior implants in group A.
  - 2- There is a significant difference between vertical and oblique loads between posterior implants in group B.
- There is a significant difference between both groups under both vertical and oblique loads regarding posterior implants

## Discussion

Prosthetic treatment for completely edentulous patients shows great variation and that depends on several factors. The huge improvement in technology of dental implants has made the replacement of missing teeth with endo-osseous implants the standard care and an implant-supported prosthesis as the first line of treatment (16).

The treatment of the atrophic edentulous maxilla is more complicated and requires more elective procedures than are necessary for the mandible. Treatment protocols for implant-supported prostheses advocating the insertion of tilted implants are gaining increasing acceptance in the literature (17,18).

This study has observed the stresses generated around implants in the all-on-four treatment concept which uses the tilted implants protocols. The All-On-Four treatment concept allows the rehabilitation of an atrophic edentulous jaw in a single operation and eliminating nerve transposition and/or bone grafting procedures. Also, many biomechanical advantages are obtained by achieving a wide anteroposterior distance, providing better load distribution in the occlusal plane, avoiding a long cantilever distance, and increasing the bone-implant contact with the use of longer implants (19-21).

The two ready-made identical epoxy resin models were used to have an appropriate elastic modulus for a bone analog material (22). It was also found to produce better results than plaster models used in other studies (23). Using of mucosa simulating layer from flexible polyurethane to ensure simulation of oral environment (24).

The surgical guides that were used in this research were manufacturing using CAD-CAM technology to control implant position, angulation, and drilling depth. Virtual implant placement makes it possible to account for anatomic limitations and visualize available bone relative to the ideal position of the final restoration (25,26).

The radiographic stent was manufactured in this study to allows the placement of the implant along planned prosthetic axes during surgery. A radiographic stent allows visualizing the planned implant axis, position of the definitive prosthesis, emergence site, available space for the attachment components, and thickness of the mucosa overlying the bone. (27,28)

The canine area was selected to be the site of implantation for anterior implants. Resorbed maxilla shows the limitation of implant placement due to anatomical insufficiency especially posteriorly, this makes the canine area is preferable for implant. (29)

The second premolar area was preferred in this study for posterior implantation to avoid penetration of the maxillary sinus and consequently the need for extensive grafting. However, the first molar area may be a key for implant position since the bite force doubles in a molar area when compared to the premolar area. (30,31)

Group A in this research has posterior implants with 45 degrees of tilt while group B has posterior implants tilted by 30 degrees. This was planned according to different anatomic needs (anterior sinus wall) for different patients, and allow the use of implants with a longer length, besides reducing the extension of the cantilever by increasing the anterior-posterior (AP) distance. Furthermore, implant tilting can contribute to the anchorage of the distal implant and support primary stability. The anterior implants in both groups were planned to be placed vertically. (8, 32-34)

Straight multiunit abutments were used for anterior implants and 30 degrees angled multiunit abutments were used for posterior implants to achieve good parallelism between abutments and ensure the passive fit of fixed detachable prosthesis. (35)

In this study, the indirect fabrication technique was used via castable plastic cylinders for waxing up the metallic framework and subsequent steps of prosthesis fabrication to makes sure for the accurate passive fit of the prosthesis and reduce casting errors to minimum levels. Also, it helps to reduce fatigue fracture of the prosthesis and improve fracture resistance. (36,37)

The cantilever length was designed to be the same in both casts. This was to neglect the effect of increasing or decreasing the cantilever length on stress transmission to implants as cantilever length generate different stress pattern around implants. (38)

In this study, tunnels were made at the sites of the strain gauge installation for gaining deeper insight into the stress distribution at the implant-bone interface. (39-41)

Installation of the strain gauges was done from the top of the models because the cervical region of the implant is the site where the highest stresses occur, regardless of the type of bone and the design of the implant. (42,43)

The installation of strain gauges was done in prepared flat surfaces in the epoxy resin parallel to the long axis of the implant fixture instead of placing it directly on the root surface or implant surface because it is preferred to bond the strain gauge on a completely flat surface to minimize the possibility of obtaining incremental apparent strain that results from mounting the strain gauge on a curved surface. (44,45)

Using four strain gauges installed to the mesial, distal, buccal and palatal aspects to ensure proper recording of all the stress around the implants. (46)

The occlusal plate was fabricated in a manner to occlude with restoration to ensure equal distribution of forces on all implants and simultaneous loading on both sides of the prosthesis, so it allows to capture the force in all the implants. (47,48)

A universal testing machine was used to deliver the load in this study. It is digital and easy to use. Besides, it offers high accuracy position measurement, rapid data acquisition and full personal

computer integration. Also, it allows the determination of stresses either compressive or tensile while avoiding complications caused by the catching system of the samples. (49,50)

In this study, a bilateral vertical static load of 100 N and oblique static load of 65 N were applied (40). Strain gauge studies in implantology generally use loads varying from 20 to 300 N. (39,44 50,51)

The load is applied 10 times for each model vertically and also obliquely to ensure the reproducibility of the results and for the accuracy of the results, an interval of at least 5 minutes between each reading was given to give a chance for heat dissipation from the strain gauge sensors and to allow relief of formed strains before making the next reading. (52)

This study showed that there is no statistically significant difference between right and left implants anterior implants in the same group. These results may be due to the loading was applied in the same manner for the same group under both vertical and oblique load, also when comparing the two groups with other we observed that there was no statistically significant difference between anterior implants of both groups under both vertical and oblique loads as the load was distributed equally in the buccal, palatal, mesial and distal surfaces around each vertical implant. (53)

When comparing right and left posterior implants, we observed that there is no statistically significant difference between posterior implants of the same group under both vertical and oblique load as anterior implants were observed. (53)

However, the results of this study showed that there is a significant difference between both groups regarding posterior implants under both vertical and oblique loads. The stress is increasing in case of increasing implant angulations from 30 to 45 degrees. These results were supported by Begg et al (54), Silva et al (55), Cidade et al (56) who stated that increasing implant angulation may cause stresses to increase around implants in every condition.

On the other hand, different researches (57-59) proved that there is an unexpected decrease in stresses around 45 degrees tilted implants and they related it to decrease cantilever length of prosthesis that counteract increased stresses due to increasing angulation. However, in this study cantilever length was fixed in both models to eliminate the effect on cantilever effect.

This study showed that the least stress was found around two anterior vertical implants in comparison to the two posterior tilted implants in the same group under both vertical and oblique loads, this is supported by different studies who explained it by considering the angulations of the posterior implants and the formation of bending moments at these sites which in turn distribute load unequally around the implant causing stress concentration at cervical region of tilted implants. (53,60-62)

In the study performed by Begg et al (54) by using photoelastic analysis, it was concluded that there is a notable difference between anterior and posterior implants in the case of tilting the posterior by 45 degrees while there is no notable difference is noticed between anterior and posterior implants in case

of tilting implants by 30 degrees. The data obtained in the previous study are qualitative, unclear and no statistical analysis was performed whether these observed differences are significant.

Also, when comparing both anterior implants between two groups under both vertical and oblique load, it is founded that there is no significance between both groups regarding anterior implants. However, the mean and standard deviation were higher in group A than in Group B. This can be referred to as increasing tilt of posterior implants will increase stresses around anterior implants. Therefore, not only would the stress concentration in posterior implants be higher, but anterior implants would also be subjected to higher amounts of stress. (61,62)

When comparing both posterior implants between two groups under both vertical and oblique load, it is founded that both groups are significant regarding posterior implants. This is explained by different researchers due to increased implant angulation which will subject tilted implants to higher stresses. (55,56)

Results of this study showed that the stress was increased around implants in case of oblique loading of force more than the vertical loading by a significant difference.

These results were supported by many studies which proved that the higher stress values of the oblique loading compared to the vertical loading, could be attributed to the fact that the non-axial forces tend to cause uneven stress distribution leading to areas of higher stresses and others of low stresses. It can be concluded that occlusal contacts positioned laterally along the axis of the implant produce higher stresses around the implant and contribute to peri-implant bone resorption. (39,63-65)

## **Conclusions**

**Within the limitations of this in-vitro study, it can be concluded that:**


- Without the cantilever influence, the 45° degrees of tilting lead to more stress than 30° degrees of inclination around implants. Also increasing the tilt subject anterior implants to more stresses.
- Tilting implants will cause more stress on fixtures than placing them vertically.
- Whenever possible, avoid nonaxial loading on implants to reduce the number of forces over dental implants.




**Figure (1):** epoxy resin models



**Figure (2):** Surgical guide fit in both model

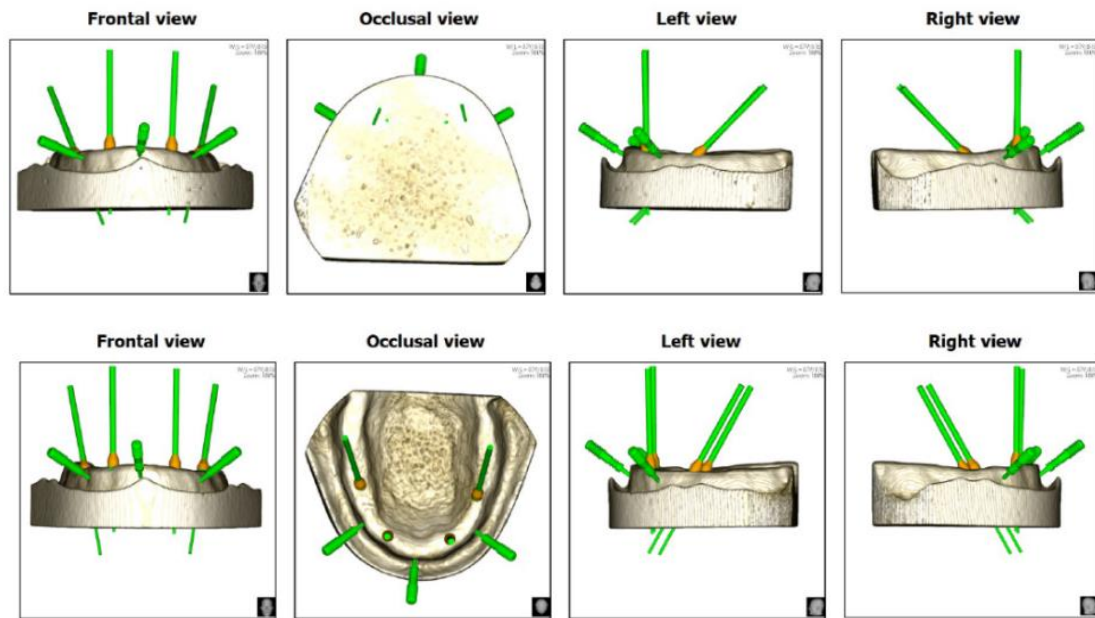

**Figure (3):** implant planning in both models.

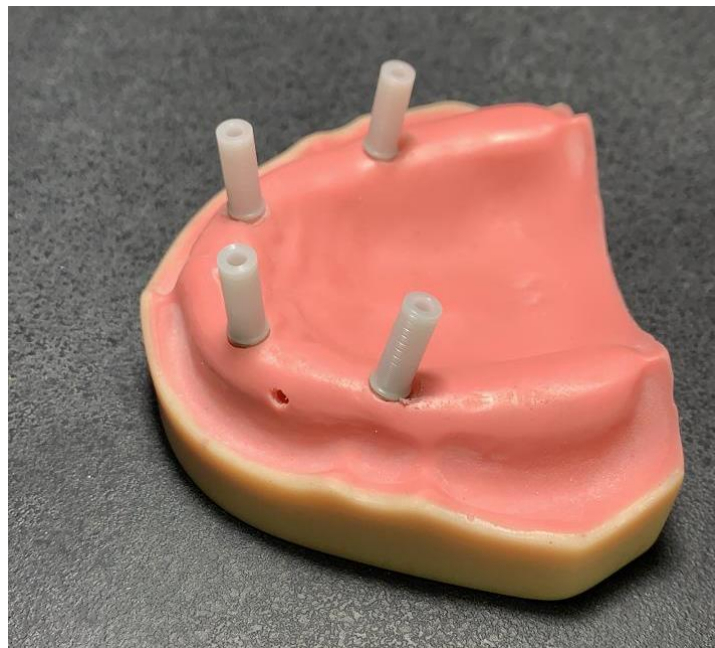


**Figure (4):** castable cylinder coping placed on abutments.




**Figure (5):** Try in of metallic framework




**Figure (6):** Conventional porcelain after finishing and polishing

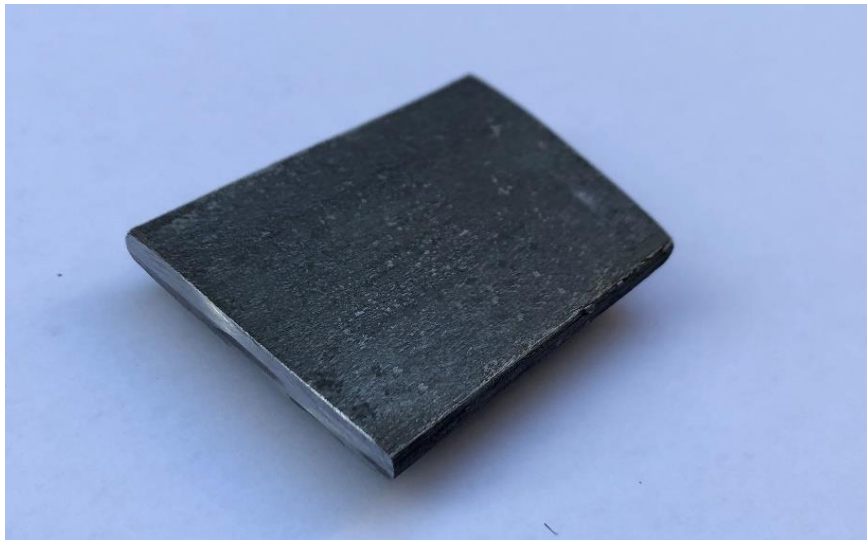

**Figure (7):** Occlusal Plate

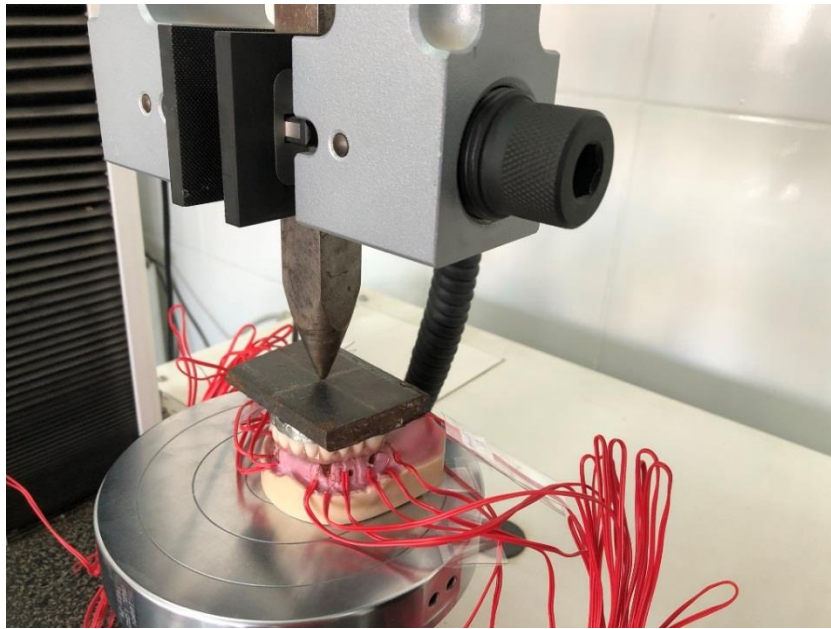

**Figure (8):** Measuring Vertical load

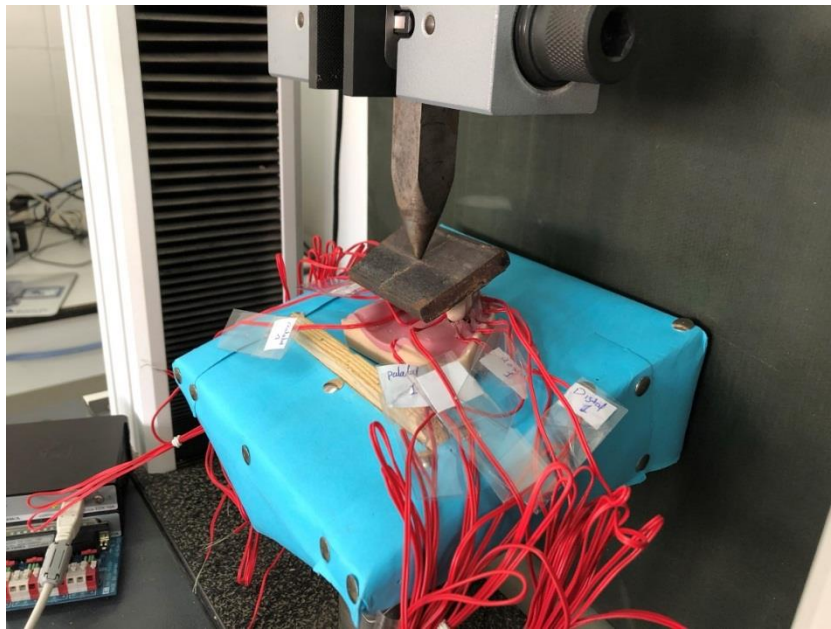

**Figure (9):** Measuring Oblique load

**Ethical approval and consent to participate**

Not Applicable

**Availability of data and material**

The authors declare that they have full control over all data and materials of this study.

**Funding**

Not Applicable

**Acknowledgments**

Not Applicable

**References**

1. Bhering CLB, Henriques SE, Girundi F, Miranda M, Vasconcellos A. Full arch implant supported oral rehabilitation to reestablish esthetic and function. *Int J Clinic Dent.* 2017; 10: 25-33.
2. El-Anwar MI, El-Zawahry MM, Ibraheem EM, Nassani MZ, ElGabry H. New dental implant selection criterion based on implant design. *Eur J Dent.* 2017; 11:186-191.
3. Mericske-Stern RD, Taylor TD, Belser U. Management of the edentulous patient. *Clinic O Imp R.* 2000; 11:108-125.
4. El-Amier N, Elsaih E, Gibreel M, El-Motaiaam H. Effect of Implant Location on Palateless Complete Overdenture Retention: An In Vitro Study. *J Oral Maxillofac Res.* 2018; 9: 1-9.
5. Aparicio C, Perales P, Rangert B. Tilted Implants as an Alternative to Maxillary Sinus Grafting: A Clinical, Radiologic, and Periotest Study. *Clin Implant Dent Relat Res.* 2001; 3:39-49.
6. Malo P, Rangert B, Nobre M. "All-on-Four" immediate-function concept with Branemark System implants for completely edentulous mandibles: a retrospective clinical study. *Clin Implant Dent Relat Res.* 2003; 5: 2-9.
7. Lyra D. All on four concept and predictability in edentulous jaws. *Clinical oral implants research.* 2018; 29:367-368.

8. Maló P, de Araújo Nobre M, Lopes A, Francischone C, Rigolizzo M. "All-on-4" immediate-function concept for completely edentulous maxillae: a clinical report on the medium (3 years) and long-term (5 years) outcomes. *Clin Implant Dent Relat Res.* 2012; 14:139-150.
9. El-Anwar MI, El-Zawahry MM, Ibraheem EM, Nassani MZ, ElGabry H. New dental implant selection criterion based on implant design. *Eur J Dent.* 2017; 11:186-191.
10. Pjetursson BE, Tan K, Lang NP, Braegger U, Egger M & Zwahlen M. A systematic review of the survival and complication rates of fixed partial dentures (FPDs) after an observation period of at least 5 years. I. Implant-supported FPDs. *Clin Oral Implants Res.* 2004; 15: 625–642.
11. Jung RE, Pjetursson BE, Glauser R, Zembic A, Zwahlen M, Lang NP. A systematic review of the 5-year survival and complication rates of implant-supported single crowns. *Clin Oral Implants Res.* 2008; 19: 119–130.
12. Abullais S, AlQahtani N, Kudyar N, Priyanka N. Success of dental implants: Must-know prognostic factors. *J Dent Imp.* 2016; 6: 44-48.
13. Abdelfattah F, Elkafrawy M, Talep F. Comparative evaluation of two different implant lengths for implant-assisted complete mandibular overdenture. *T Dent J.* 2016; 17:139–146.
14. Abdelfattah F, Elhadad F, Kashef N. Clinical and radiographic comparative study between two different types of clasps materials used in unilateral maxillary Kennedy class II removable partial denture cases. *T Dent J.* 2016; 17:119–126.
15. Abdelfattah F. Comparative Study of Two Designs of Maxillary Implant-Supported Overdentures. *Egy Dent J.* 2009; 55:1845-1856.
16. Gowd MS, Shankar T, Ranjan R, Singh A. Prosthetic Consideration in Implant-supported Prosthesis: A Review of Literature. *J Int Soc Prev Community Dent.* 2017;7(Suppl 1):1-7.
17. Taruna M, Chittaranjan B, Sudheer N, Tella S, Abusaad M. Prosthodontic perspective to all-on-4® concept for dental implants. *J Clin Diagn Res.* 2014; 8:16-19.
18. Sadowsky SJ. Treatment considerations for maxillary implant overdentures: a systematic review. *J Prosthet Dent.* 2007; 97:340-348.
19. Penarrocha-Diago M, Zaragoza-Alonso R, Soto-Penalosa D, Ticare Consensus M. Consensus statements and clinical recommendations on treatment indications, surgical procedures, prosthetic protocols, and complications following All-On-4 standard treatment. *J Clin Exp Dent.* 2017; 9:712-715.
20. Peñarrocha-Oltra D, Candel-Martí E, Ata-Ali J, Peñarrocha-Diago M. Rehabilitation of the atrophic maxilla with tilted implants: review of the literature. *J Oral Implantol.* 2013; 39:625-632.

21. Wentaschek S, Lehmann KM, Scheller H, Weibrich G, Behneke N. Polygonal Area of Prosthesis Support with Straight and Tilted Dental Implants in Edentulous Maxillae. *Int J Prosthodont*. 2016; 29:245-252.
22. Lee CK, Karl M, Kelly JR. Evaluation of test protocol variables for dental implant fatigue research. *Dental materials: official publication of the Academy of Dental Materials*. 2009; 25:1419-25.
23. Camardella L, Breuning H, Vilella OV. Are there differences between comparison methods used to evaluate the accuracy and reliability of digital models? *Dental Press Journal of Orthodontics*. 2017; 22:65-74.
24. Ali H, Roodabeh K, Seyed G, Noorazar, Masoud H-B, Mehran H, Neda Y. Evaluation of strain in mandibular denture-supporting area in three different occlusal schemes during jaw movements. *J Dent Res*. 2017; 12:18-25.
25. Fortin T, Bosson JL, Coudert JL, Isidori M. Reliability of preoperative planning of an image-guided system for oral implant placement based on 3-dimensional images: an in vivo study. *Int J Oral Maxillofac Implants*. 2003; 18:886-893.
26. Colombo M, Mangano C, Mijiritsky E, Krebs M, Hauschild U, Fortin T. Clinical applications, and effectiveness of guided implant surgery: a critical review based on randomized controlled trials. *BMC oral health*. 2017; 17:150-159.
27. Kulkarni P, Bulbule N, Kakade D, Hakepatil N. Radiographic Stents and Surgical Stents in Implant Placements: An Overview. *IGCRR*. 2019; 11:11-15.
28. Pal US, Chand P, Dhiman NK, Singh RK, Kumar V. Role of surgical stents in determining the position of implants. *Natl J Maxillofac Surg*. 2010; 1:20-23.
29. Joseph YK, Kitichai R, Kiyotaka U, Joh CK. Dimensions of Peri-Implant Mucosa: An Evaluation of Maxillary Anterior Single Implants in Humans. *J Periodontol*. 2003; 74:557-62.
30. Al-Ghafli SA, Michalakis KX, Hirayama H, Kang K. The in vitro effect of different implant angulations and cyclic dislodgement on the retentive properties of an overdenture attachment system. *J Prosthet Dent*. 2009; 102:140-147.
31. Widbom C, Soderfeldt B, Kronstrom M. A retrospective evaluation of treatments with implant-supported maxillary overdentures. *Clin Implant Dent Relat Res*. 2005; 7:166-172.
32. Joseph YK, Kitichai R, Kiyotaka U, Joh CK. Dimensions of Peri-Implant Mucosa: An Evaluation of Maxillary Anterior Single Implants in Humans. *J of Periodontol*. 2003; 74:557-562.
33. Nawar N, Thabet Y. Clinical and radiographic assessment of different occlusal schemes in "All on 4" concept. *Egy D J*. 2018; 64:2785-2792.

- 34.Lopes A, Maló P, de Araújo Nobre M, Sanchez-Fernández E. The NobelGuide® All-on-4® Treatment Concept for Rehabilitation of Edentulous Jaws: A Prospective Report on Medium- and Long-Term Outcomes. *Clin Implant Dent Relat Res.* 2015; 17 Suppl 2:406-416.
- 35.Buzayan MM, Yunus NB. Passive Fit in Screw Retained Multi-Unit Implant Prosthesis Understanding and Achieving: A Review of the Literature. *J Indian Prosthodont Soc.* 2014; 14:16-23.
- 36.Ganz SD, Desai N, Weiner S. Marginal integrity of direct and indirect castings for implant abutments. *Int J Oral Maxillofac Implants.* 2006; 21:593-599.
- 37.Chang TL, Maruyama C, White SN, Son S, Caputo AA. Dimensional accuracy analysis of implant framework castings from 2 casting systems. *Int J Oral Maxillofac Implants.* 2005; 20:720-725.
- 38.Bevilacqua M, Tealdo T, Menini M, Pera F, Mossolov A, Drago C, et al. The influence of cantilever length and implant inclination on stress distribution in maxillary implant-supported fixed dentures. *J Prosth Dent.* 2011; 105:5-13.
- 39.Hesham S, Abdelfattah F, Elguindy M. Comparative study of strain analysis between different designs of maxillary implant assisted overdenture. Thesis submitted at Prosthodontics Department, Faculty of Dentistry, Tanta University. 2019.
- 40.Ibrahim AB, El-sheikh MM, El-gendy MNM. comparison between stress distribution around straight and tilted posterior dental implant with different lengths (in vitro study). *M J Dent.* 2017; 12:12-21.
- 41.Karl M, Wichmann MG, Winter W, Graef F, Taylor TD, Heckmann SM. Influence of fixation mode and superstructure span upon strain development of implant fixed partial dentures. *J Prosthodont.* 2008; 17:3-8.
- 42.Dahab I, El-Gendy AA, Eltorkey IR. In vitro stress analysis study of different prosthetic options using single posterior implant for management of mandibular unilateral distal extension saddle. *Tanta Dent J.* 2015; 12:7-15.
- 43.Tada S, Stegaroiu R, Kitamura E, Miyakawa O, Kusakari H. Influence of implant design and bone quality on stress/strain distribution in bone around implants: a 3-dimensional finite element analysis. *Int J Oral Maxillofac Implants.* 2003; 18:357-368.
- 44.Akca K, Cehreli MC, Iplikcioglu H. A comparison of three-dimensional finite element stress analysis with in vitro strain gauge measurements on dental implants. *Int J Prosthodont.* 2002; 15:115-121.
- 45.El-Gendy AA. Micro-Strain Evaluation of Different Implant Positions Supporting Mandibular Bilateral Distal Extension Partial Over Denture. *Tanta Dent J.* 2007; 4:39-46.

- 46.Kanazawa M, Minakuchi S, Hayakawa I, Hirano S, Uchida T. In vitro study of reduction of stress transferred onto tissues around implants using a resilient material in maxillary implant overdentures. *J Med Dent Sci.* 2007; 54:17-23.
- Magdy EM, El Sayed. Stress analysis study of two treatment modalities rehabilitating distal extension cases with few remaining natural teeth. *C D J.* 2008; 24:379-393.
- 47.Elsyad M. Effect of different attachments designs used for implant assisted mandibular distal extension RPD. An in vitro study of stresses transmitted to abutment teeth. *Mans J Dent.* 2014; 1:124-30.
- 48.Hegazy SA, Elshahawi IM, Elmotayam H. Stresses induced by mesially and distally placed implants to retain a mandibular distal-extension removable partial overdenture: a comparative study. *Int J Oral Maxillofac Implants.* 2013; 28:403-407.
- 49.Tang X, Nakamura T, Usami H, Wakabayashi K, Yatani H. Effects of multiple firings on the mechanical properties and microstructure of veneering ceramics for zirconia frameworks. *J Dent.* 2012; 40:372-380.
- 50.Wanderley de Abreu C, Vasconcellos LG, Balducci I, Nishioka R. A comparative study of microstrain around three-morse taper implants with machined and plastic copings under axial loading. *Braz J Oral Sci.* 2016; 9:11-15.
- 51.Seong WJ, Koriath TW, Hodges JS. Experimentally induced abutment strains in three types of single-molar implant restorations. *J Prosthet Dent.* 2000; 84: 318-326.
- 52.Cekic C, Akca K, Cehreli MC. Effects of attachment design on strains around implants supporting overdentures. *Quintessence international.* 2007; 38:291-297.
- 53.Naini R, Nokar S, Borghei H, Alikhasi M. Tilted or Parallel Implant Placement in the Completely Edentulous Mandible? A Three-Dimensional Finite Element Analysis. *Int J Oral Maxillofac Implants.* 2011; 26:776-781.
- 54.Begg T, Geerts G, Gryzagoridis J. Stress Patterns Around Distal Angled Implants in the All-on-Four Concept Configuration. *Int J Oral Maxillofac Implants.* 2009; 24:663-671.
- 55.Silva G, Mendonça J, Lopes L, Landre Júnior J. Stress Patterns on Implants in Prostheses Supported by Four or Six Implants: A Three-Dimensional Finite Element Analysis. *Int J Oral Maxillofac Implants.* 2010; 25:239-246.
- 56.Cidade C, Olate S, Pozzer L, Pimentel M, Nobilo M, Barbosa JRD. Stress Analysis in Maxillary All-On-Four Model. *Int J Odontostomatology.* 2015; 9:205-211.

- 57.Gümrükçü Z, Korkmaz YT. Influence of implant number, length, and tilting degree on stress distribution in atrophic maxilla: a finite element study. *Med Bio Eng Comp.* 2018; 56:979-989.
- 58.Kilic E, Doganay O. Evaluation of Stress in Tilted Implant Concept with Variable Diameters in the Atrophic Mandible: Three-Dimensional Finite Element Analysis. *J Oral Implantol.* 2020; 46:19-26.
- 59.Ozan O, Kurtulmus-Yilmaz S. Biomechanical Comparison of Different Implant Inclinations and Cantilever Lengths in All-on-4 Treatment Concept by Three-Dimensional Finite Element Analysis. *Int J Oral Maxillofac Implants.* 2018; 33:64-71.
- 60.Canay S, Hersek N, Akpınar I, Aşık Z. Comparison of stress distribution around vertical and angled implants with finite-element analysis. *Quintessence international.* 1996; 27:591-598.
- 61.Özdemir Doğan D, Polat NT, Polat S, Şeker E, Gül EB. Evaluation of "all-on-four" concept and alternative designs with 3D finite element analysis method. *Clin Implant Dent Relat Res.* 2014; 16:501-510.
- 62.Deste G, Durkan R. Effects of all-on-four implant designs in mandible on implants and the surrounding bone: A 3-D finite element analysis. *Niger J Clin Pract.* 2020; 23:456-463.
- 63.Saad A, Eskander AE, Elkerdawy MW, Fawzy SA. Stress Distribution with Different Implant Dimensions in Implant-Supported Partial Overdentures. *J Res Prac Dent.* 2014; 2014:6-17.
- 64.Barbier L, Vander Sloten J, Krzesinski G, Schepers E, Van der Perre G. Finite element analysis of non-axial versus axial loading of oral implants in the mandible of the dog. *J Oral Rehabil.* 1998; 25:847-58.
- 65.Forero L, Castilla R, González Estrada O. Effect of force angle on the strain distribution of osseointegrated dental implants. *J Phys Conf Ser.* 2019; 1388:12-22.